

Installation Guide

Display Mount for Philips MP90 CPU


The purpose of this guide is to:

1. Describe attachment of Display Mount to CPU (pages 1 – 3).
2. Describe mounting of display (page 4).
3. Describe tilt and tilt tension adjustments (page 5).

Parts Reference


The following parts and hardware are included with this installation kit (hardware not shown):




Item #	Description	Qty
1	Display Mount	1
2	M3 x 12mm PHMS	5
3	Spacer, Camlock Lever	1
4	#4 x 3/8" Flat Head Machine Screw (FHMS)	1
5	9/64" Hex Wrench	1
6	Display Mounting Kit (includes instructions)	1
7	Spacer, 15" Display (see page 4)	1
8	Spacer, 17" Display (see page 4)	1


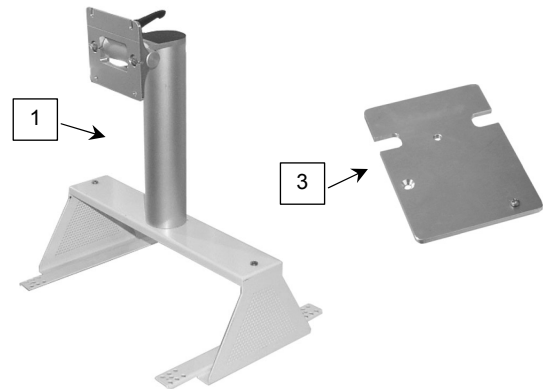


Tools Required: Small and medium-tipped Phillips screwdrivers (not provided), and 9/64" hex wrench (provided).

Attaching Mount to CPU

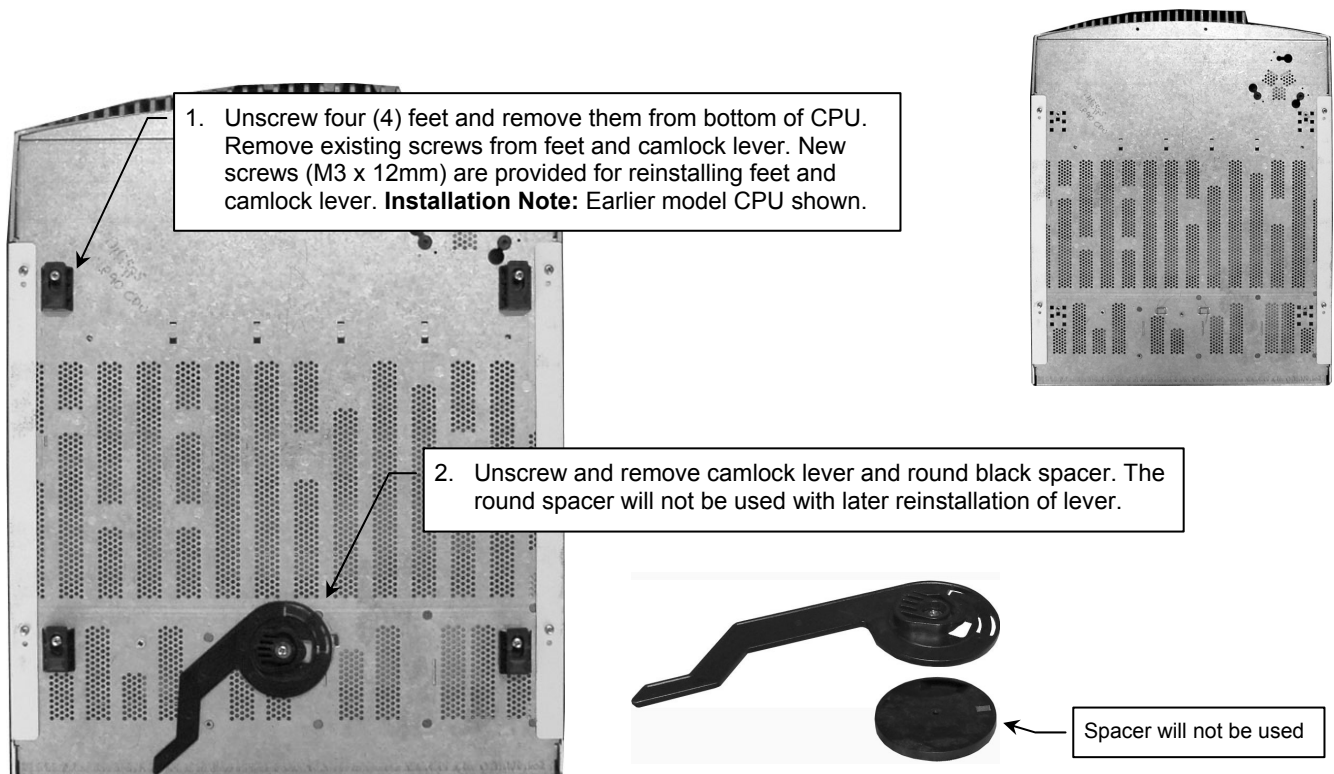

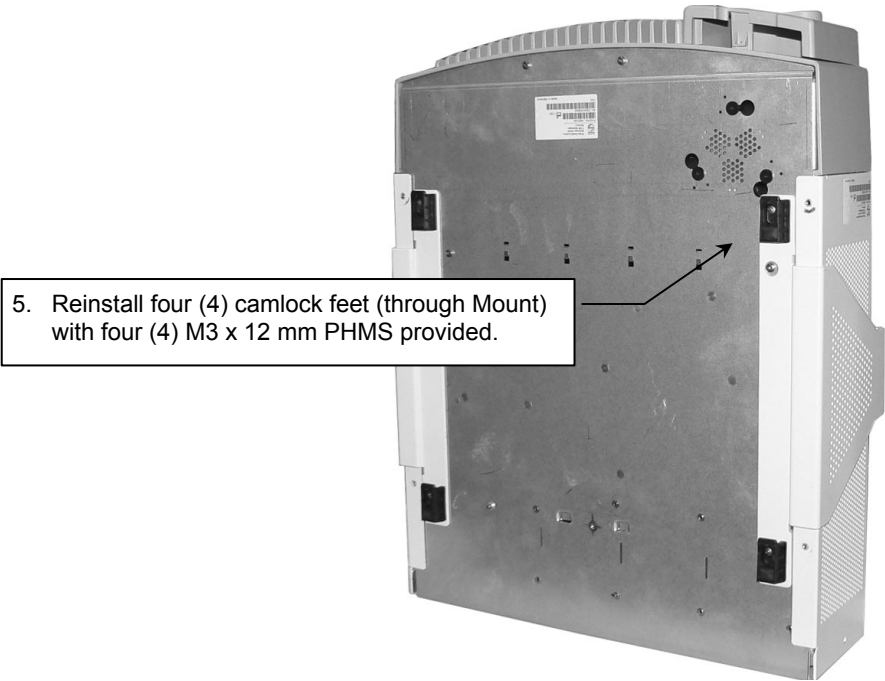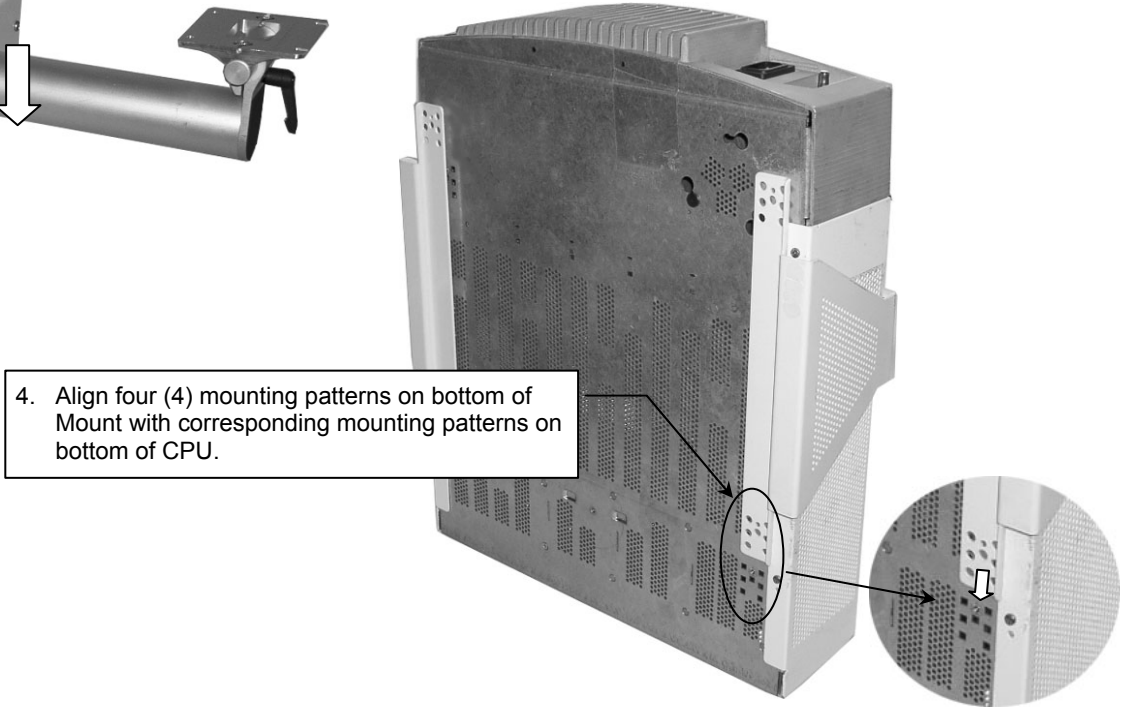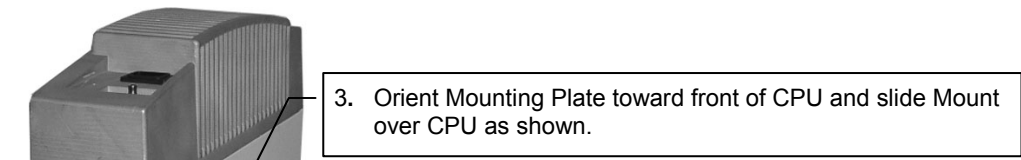

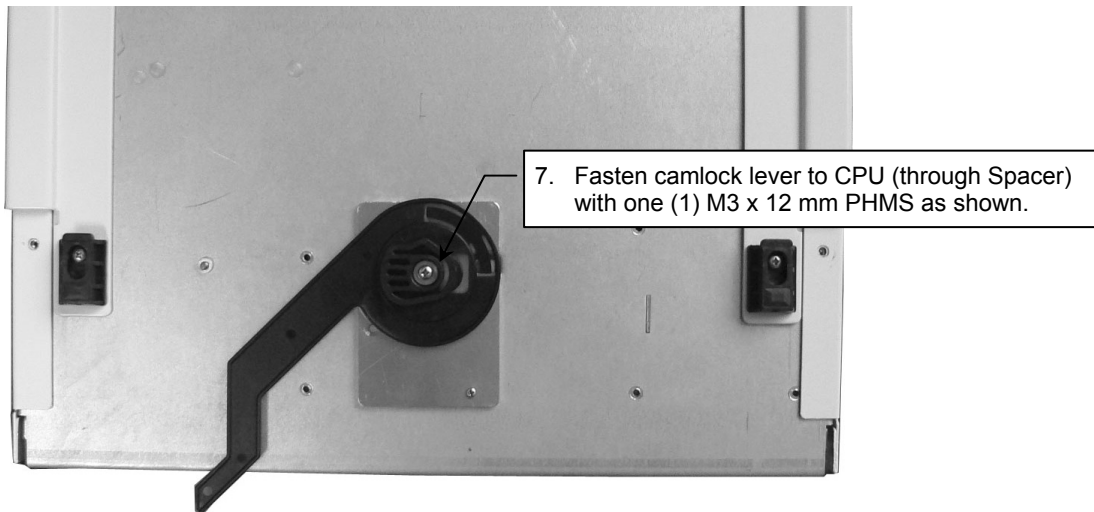
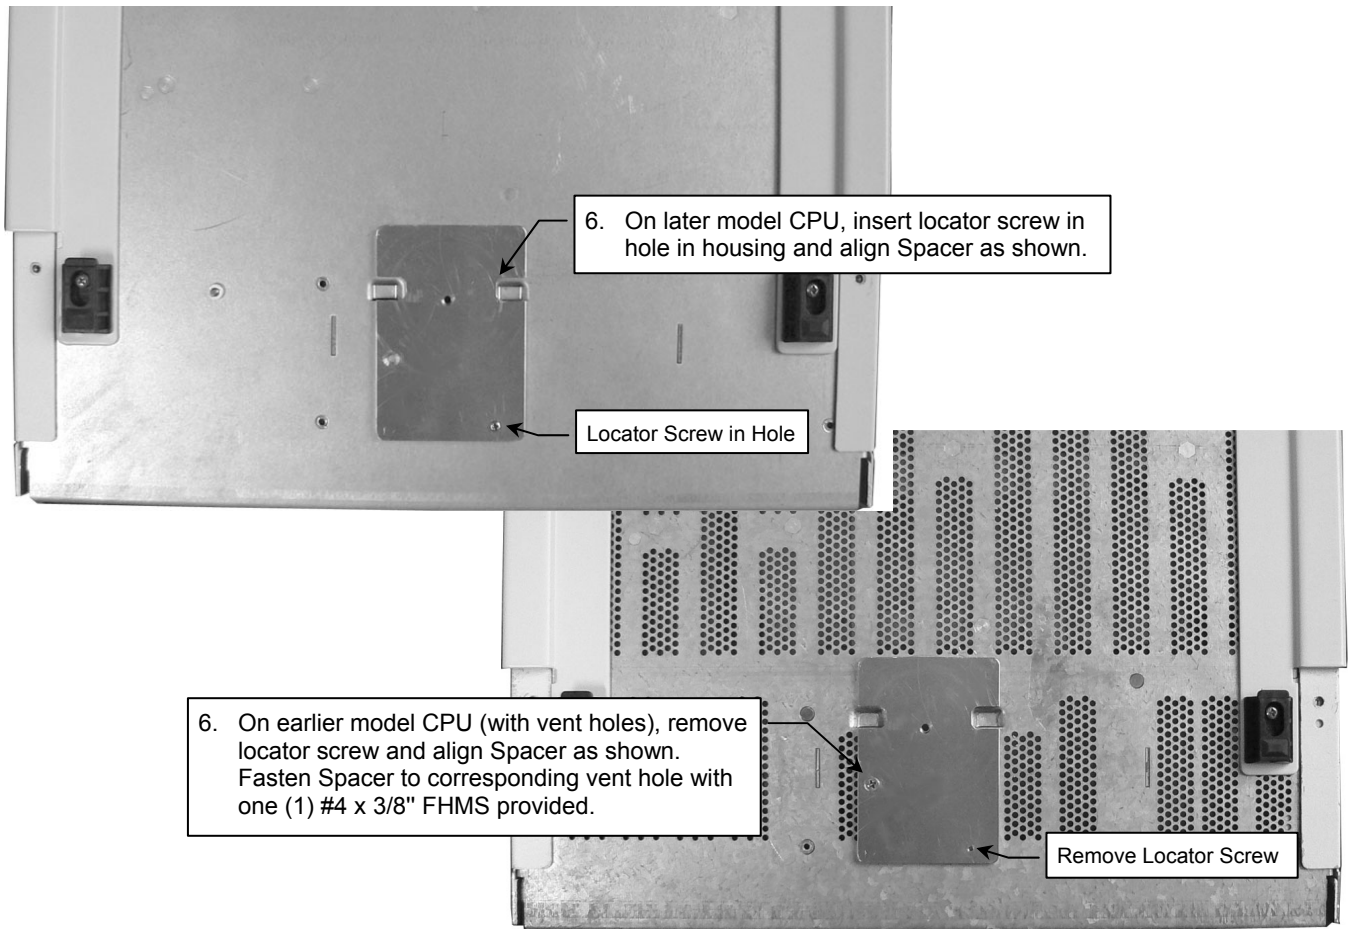


8. Mount CPU in camlock rails according to Philips installation instructions.

Mounting the Flat Panel Display

See installation guide (DU-FLP-0002-17) included with "Mounting Kit for 75/100mm VESA® Compatible Flat Panel Displays". This mounting kit provides an assortment of hardware for a wide variety of display-mounting applications.

Installation Note: A Spacer (provided) is required for mounting either an M8031B (15") or M8033C (17") display. Insert appropriate Spacer and mount display as shown below. **15" display:** Use M4 pan head machine screws from *Mounting Kit for 75/100 VESA Compatible Flat Panel Displays*. **17" display:** Use M4 pan head machine screws plus VESA Mounting Adapter from *Mounting Kit for 75/100 VESA Compatible Flat Panel Displays*.

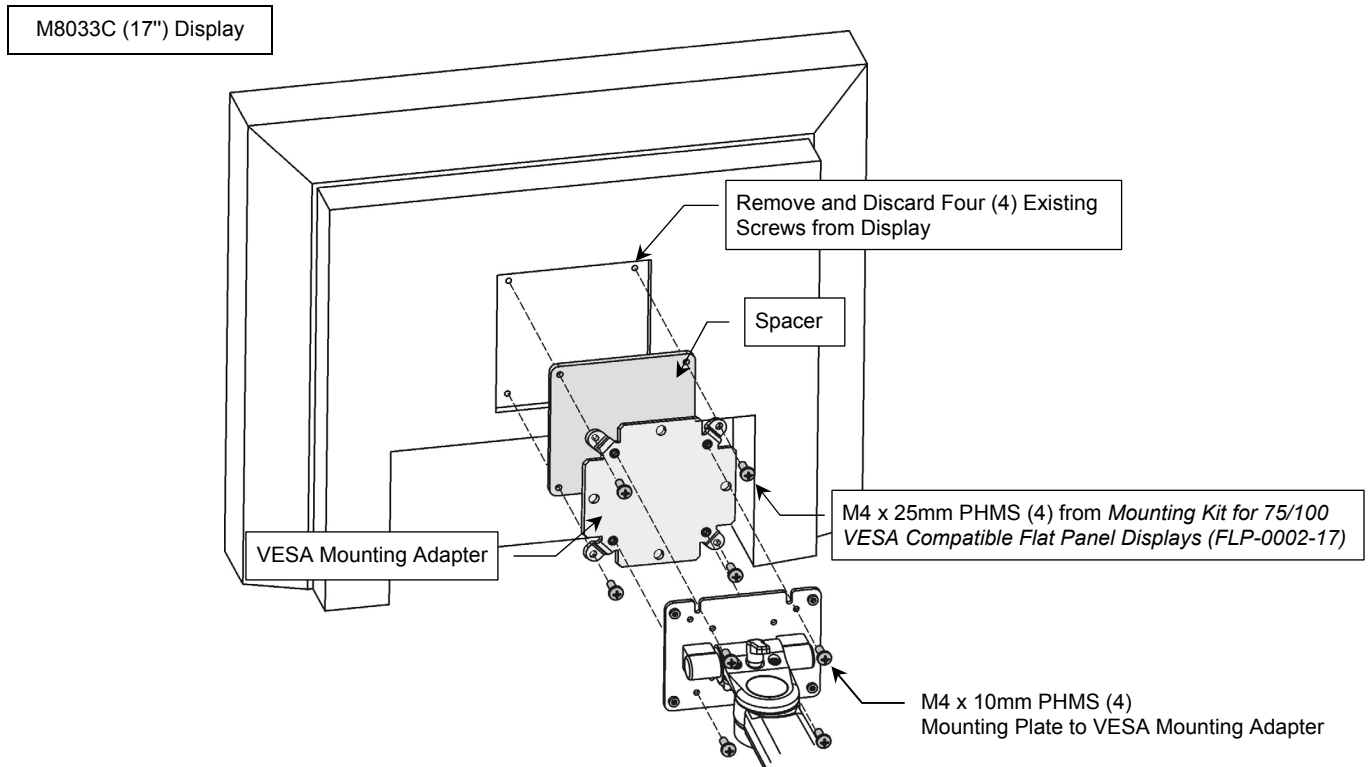
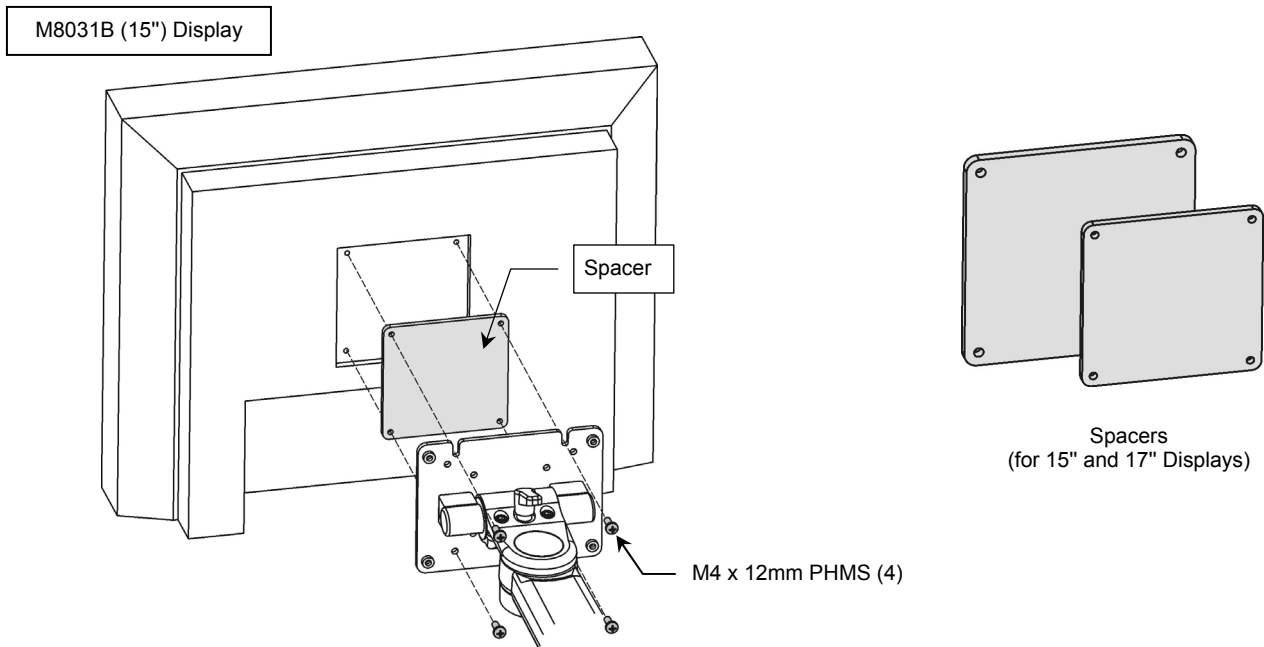


Adjusting Tilt and Tilt Tension

Tilt Tension: Adjust overall tilting tension by evenly tightening or loosening the two (2) Tension Adjustment Screws with the 9/64" hex wrench provided. Once the overall tilt tension is set, use the Tilt Adjustment Lever to fine tune/lock the tilt position.

Tilt Adjustment: Turn the Tilt Adjustment Lever counterclockwise (CCW) to loosen. Lever provides ratchet-style adjustment (see **Note** below). Grasp the display and tilt to desired angle. Turn Tilt Adjustment Lever clockwise (CW) to tighten and lock position.

Note: The Tilt Adjustment Lever is a multi-position clamping lever that operates by lifting, rotating, and releasing the handle.

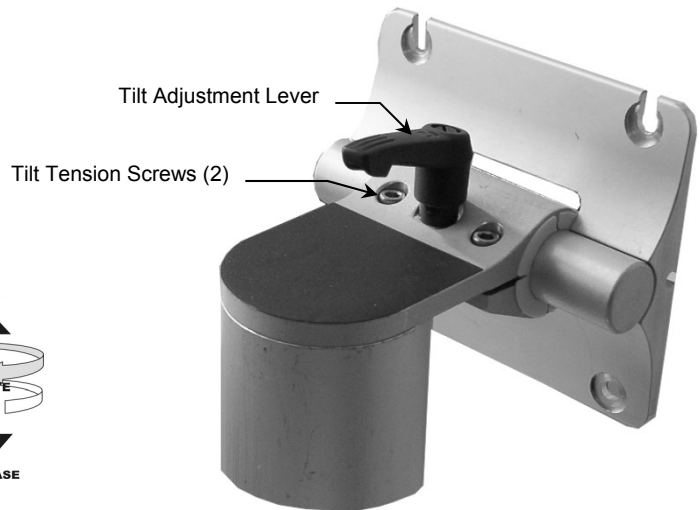

Routine Maintenance

Periodically inspect all hardware associated with the mounting system. Tighten or adjust as necessary for optimal operation and safety.

Cleaning the Mounting Assembly

1. The mounting assembly may be cleaned with most mild, non-abrasive solutions commonly used in the hospital environment (e.g. diluted bleach, ammonia, or alcohol solutions).
2. The surface finish will be permanently damaged by strong chemicals and solvents such as acetone and trichloroethylene.
3. Do not use steel wool or other abrasive material to clean the mounting assembly.
4. Damage caused by the use of unapproved substances or processes will not be covered by warranty. We recommend testing of any cleaning solution on a small area of the arm that is not visible to verify compatibility.
5. Do not submerge or allow liquids to enter the arm. Wipe any cleaning agents off of the arm immediately using a water-dampened cloth. Dry the arm thoroughly after cleaning.

CAUTION: GCX makes no claims regarding the efficacy of the listed chemicals or processes as a means for controlling infection. Consult your hospital's infection control officer or epidemiologist. To clean or sterilize mounted instruments or accessory equipment, refer to the specific instructions delivered with those products.