


# Standardize your technology and keep up with innovation

## The problem: Disconnected and underutilized patient monitoring systems

- Keeping up with constant change in technology with clinical adoption.
- Increased security risk with outdated systems.
- Technical confidence in supporting and maintaining system integration.
- Disconnect between technical capabilities and clinical user requirements.
- Unplanned and unpredictable expenditure requests may require tradeoffs and reprioritization.

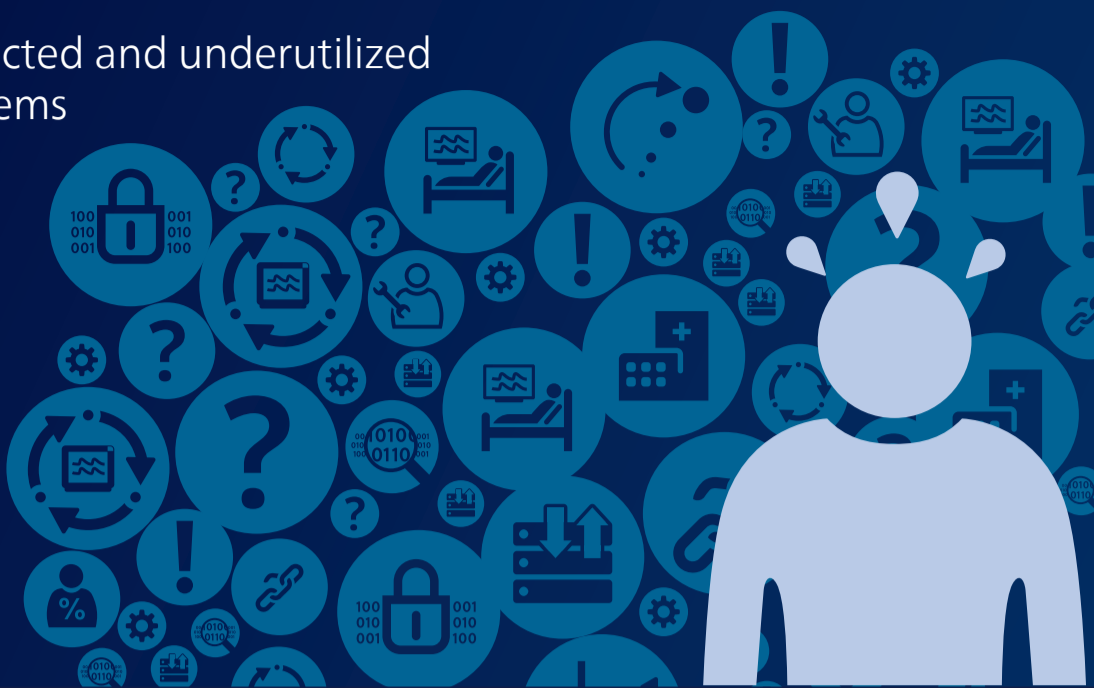

## The solution:

### Enterprise Monitoring as a Service (EMaaS)

**Provides** technology standardization using repeatable processes while driving digitization.

**Relieves** the burden of technology management with a flexible level of system support and security.

**Facilitates** rapid adoption of modern clinical monitoring technologies.

**Helps reduce** data flow disruptions with uptime commitments and security patching to avoid preventable breaches.

**Informs** operational efficiency efforts with data-driven performance analytics.

**Provides flexibility** and greater system adaptability to meet changing needs and priorities.



The shared risk model enables hospitals to access up-to-date monitoring capabilities that are aligned to your performance and growth goals – without the traditional burden of equipment management.



- 1 Baseline assessment to align the solution to your needs.
- 2 Standardization to establish hospital-wide adoption and consistency.
- 3 Ongoing optimization to support achieving your goals.

## Proven results\*



**13,331 in potential hours saved annually** through improvements from workflow changes and automation.

**8-hours daily time savings** related to automated measurement and export (wavestrip).

**5 minutes to 3.9 seconds** decrease in time spent on low-value tedious tasks during patient transport.

**90% staff satisfaction** improvement with Patient Monitoring System.

Technology decision makers, to learn more about Enterprise Monitoring as a Service (EMaaS), visit [www.philips.com/emaas](http://www.philips.com/emaas) or contact your Philips representative.



\* Results from baseline and post time and motion studies conducted by Philips and customer internal teams in the high-acuity units (ED, TICU, CCU) of one Florida hospital as well as other acuity level units. Other results from surveys conducted pre- and post-Philips installation of patient monitoring system at one Florida hospital. Results are from one Florida hospital, actual results for other health systems may vary.