


Installation Note

Installing the Fix Mount for IntelliVue Patient Monitors

This installation note describes the installation procedure for the Fix Mount for the IntelliVue MP20/30, MP40/50 and MP60/70 patient monitors.

Contents of the Fix Mount Kit

The fix mount kit contains the fix mount and two release knob covers. One for MP20-50 (white) and one for MP60/70 (grey).

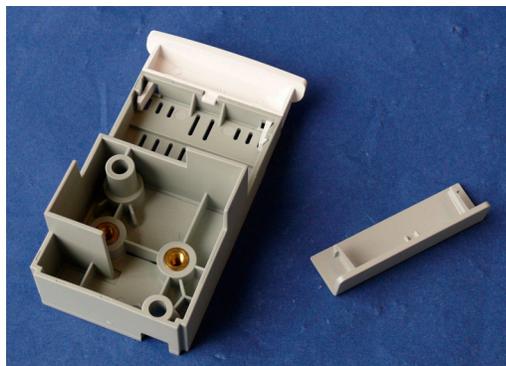



Installation Procedure for MP20/30

NOTE MP20 monitors (M8001A) with a serial number < DE42601212 and MP30 monitors (M8002A) with a serial number < DE42602155 do not allow the use of a fix mount.

- 1 Press the quick release knob down and release the lock with a small screwdriver. You can now pull out the knob.



- 2 Remove the two screws securing the quick mount, press down the quick mount release mechanism and pull the mount out of the slot in the monitor.

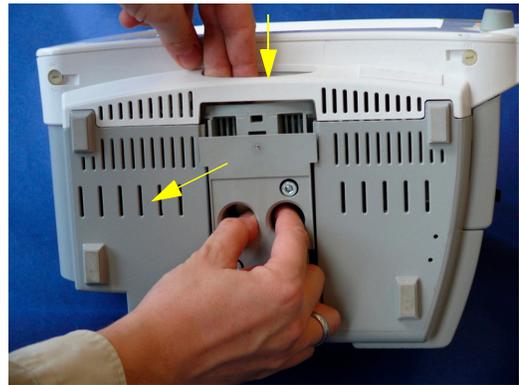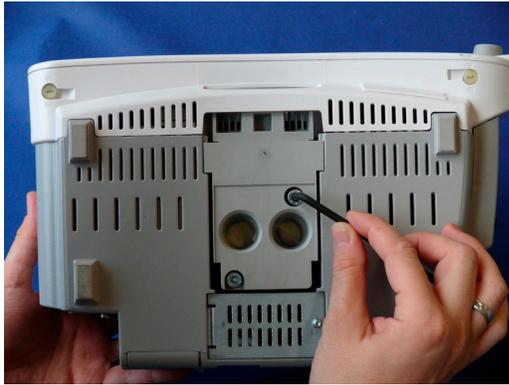

- 3 Insert the Fix Mount with the white release knob cover and secure it with two screws.



- 4 Perform the Visual and Power On Tests as described in the *Testing and Maintenance* section of your service guide.

Installation Procedure for MP40/50


- 1 Remove the two screws securing the quick mount.



- 2 Remove the battery from the battery compartment.



- 3 Remove the four screws at the back of the monitor, the lower ones first.

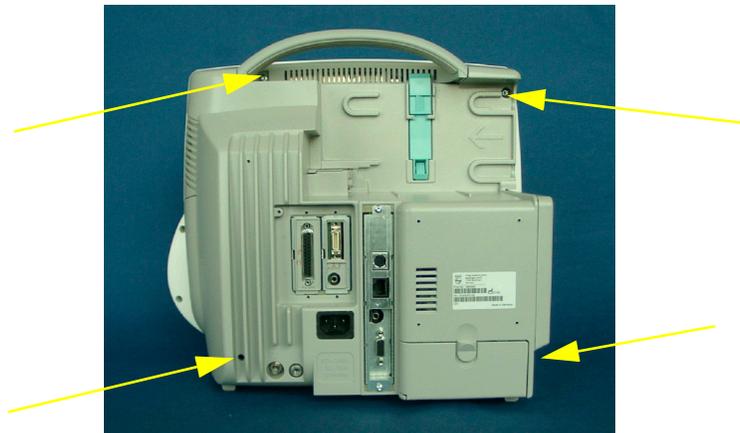

NOTE Hold on to the display when loosening the screws so the display does not fall off.


- 4 Pull off the front housing. Do not pull the display off completely, only tilt it to the front, because otherwise the flex panel adapter could be damaged.



Reassembly Note: Make sure the metal sheet on the back of the display is inserted into the noses of the monitor rear housing when reassembling the two halves.



- 5 Depending on the version of your monitor, unscrew the screws holding the flex panel adapter cable and pull off the flex cable carefully towards you or unscrew the panel adapter board and disconnect the board..

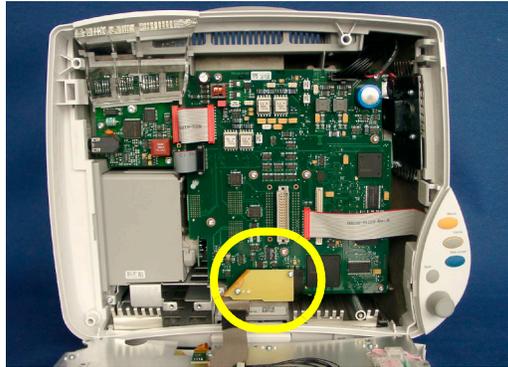

Old LG-Philips/3M Version - Remove Flex Panel Adapter Cable





New Sharp/ELO Version - Remove Panel Adapter Board




Black Spacer is attached to main board with one screw

- 6 Remove the white plastic frame from the monitor rear chassis by releasing the five snaps in the rear chassis. You can use a flat-tipped screw driver to do this.

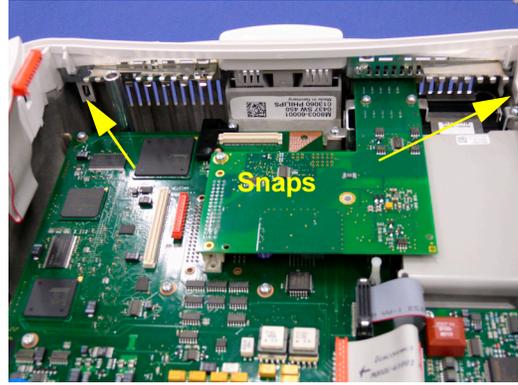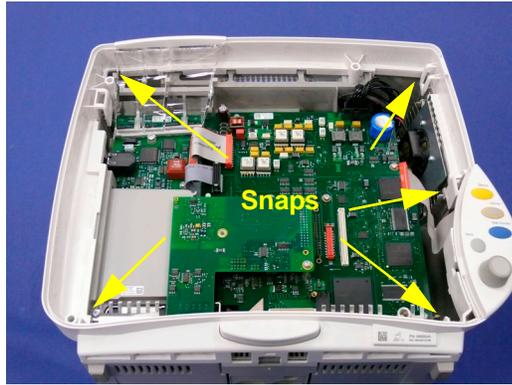


Bottom Edge of Housing


Reassembly Note: When reassembling the frame, make sure the navigation point assembly contacts are not bent and are positioned correctly inside the housing.

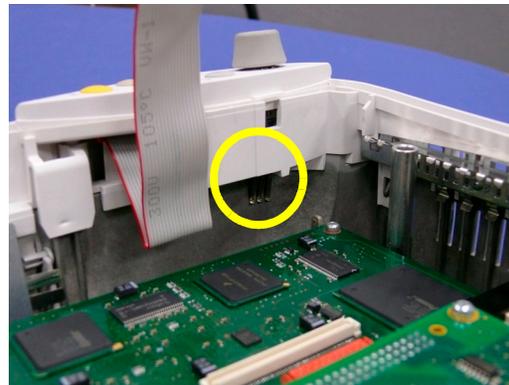

7 Pull out the quick mount.

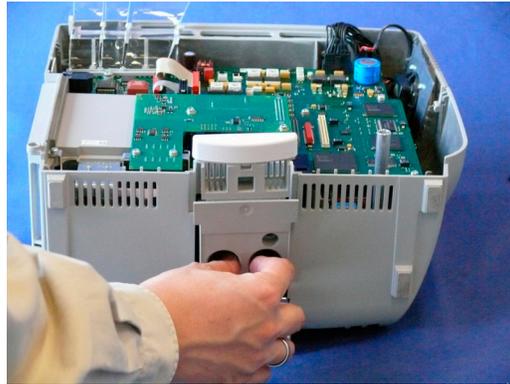

8 Insert the fix mount with the white release knob cover and secure it with two screws.

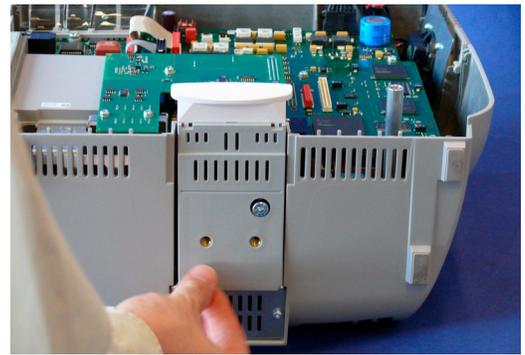

9 Reassemble the monitor by performing steps 2-6 in reverse order.




- 10 Perform the Visual, Power On and Safety Tests as described in the *Testing and Maintenance* section of your service guide.

Installation Procedure for MP60/70


- 1 Loosen the two screws securing the quick mount and pull out the quick mount



- 2 The fix mount is delivered with a white release knob cover. Remove this cover and replace it with the grey cover from your fix mount kit.

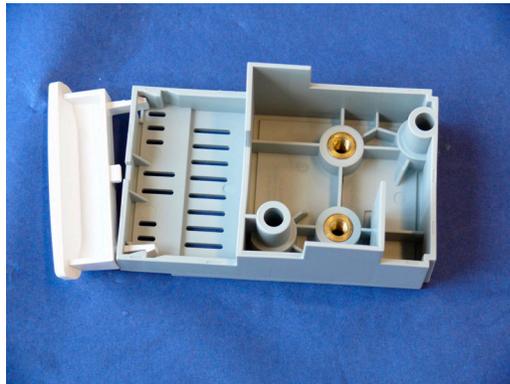

- 3 Insert the fix mount and secure it with two screws.

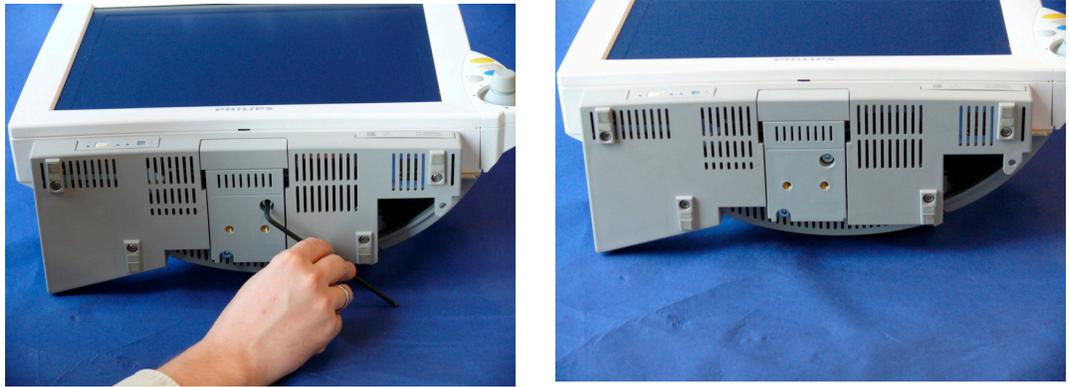

- 4 Perform the Visual and Power On Tests as described in the *Testing and Maintenance* section of your service guide.

